




WT-710

Worltech, Inc.

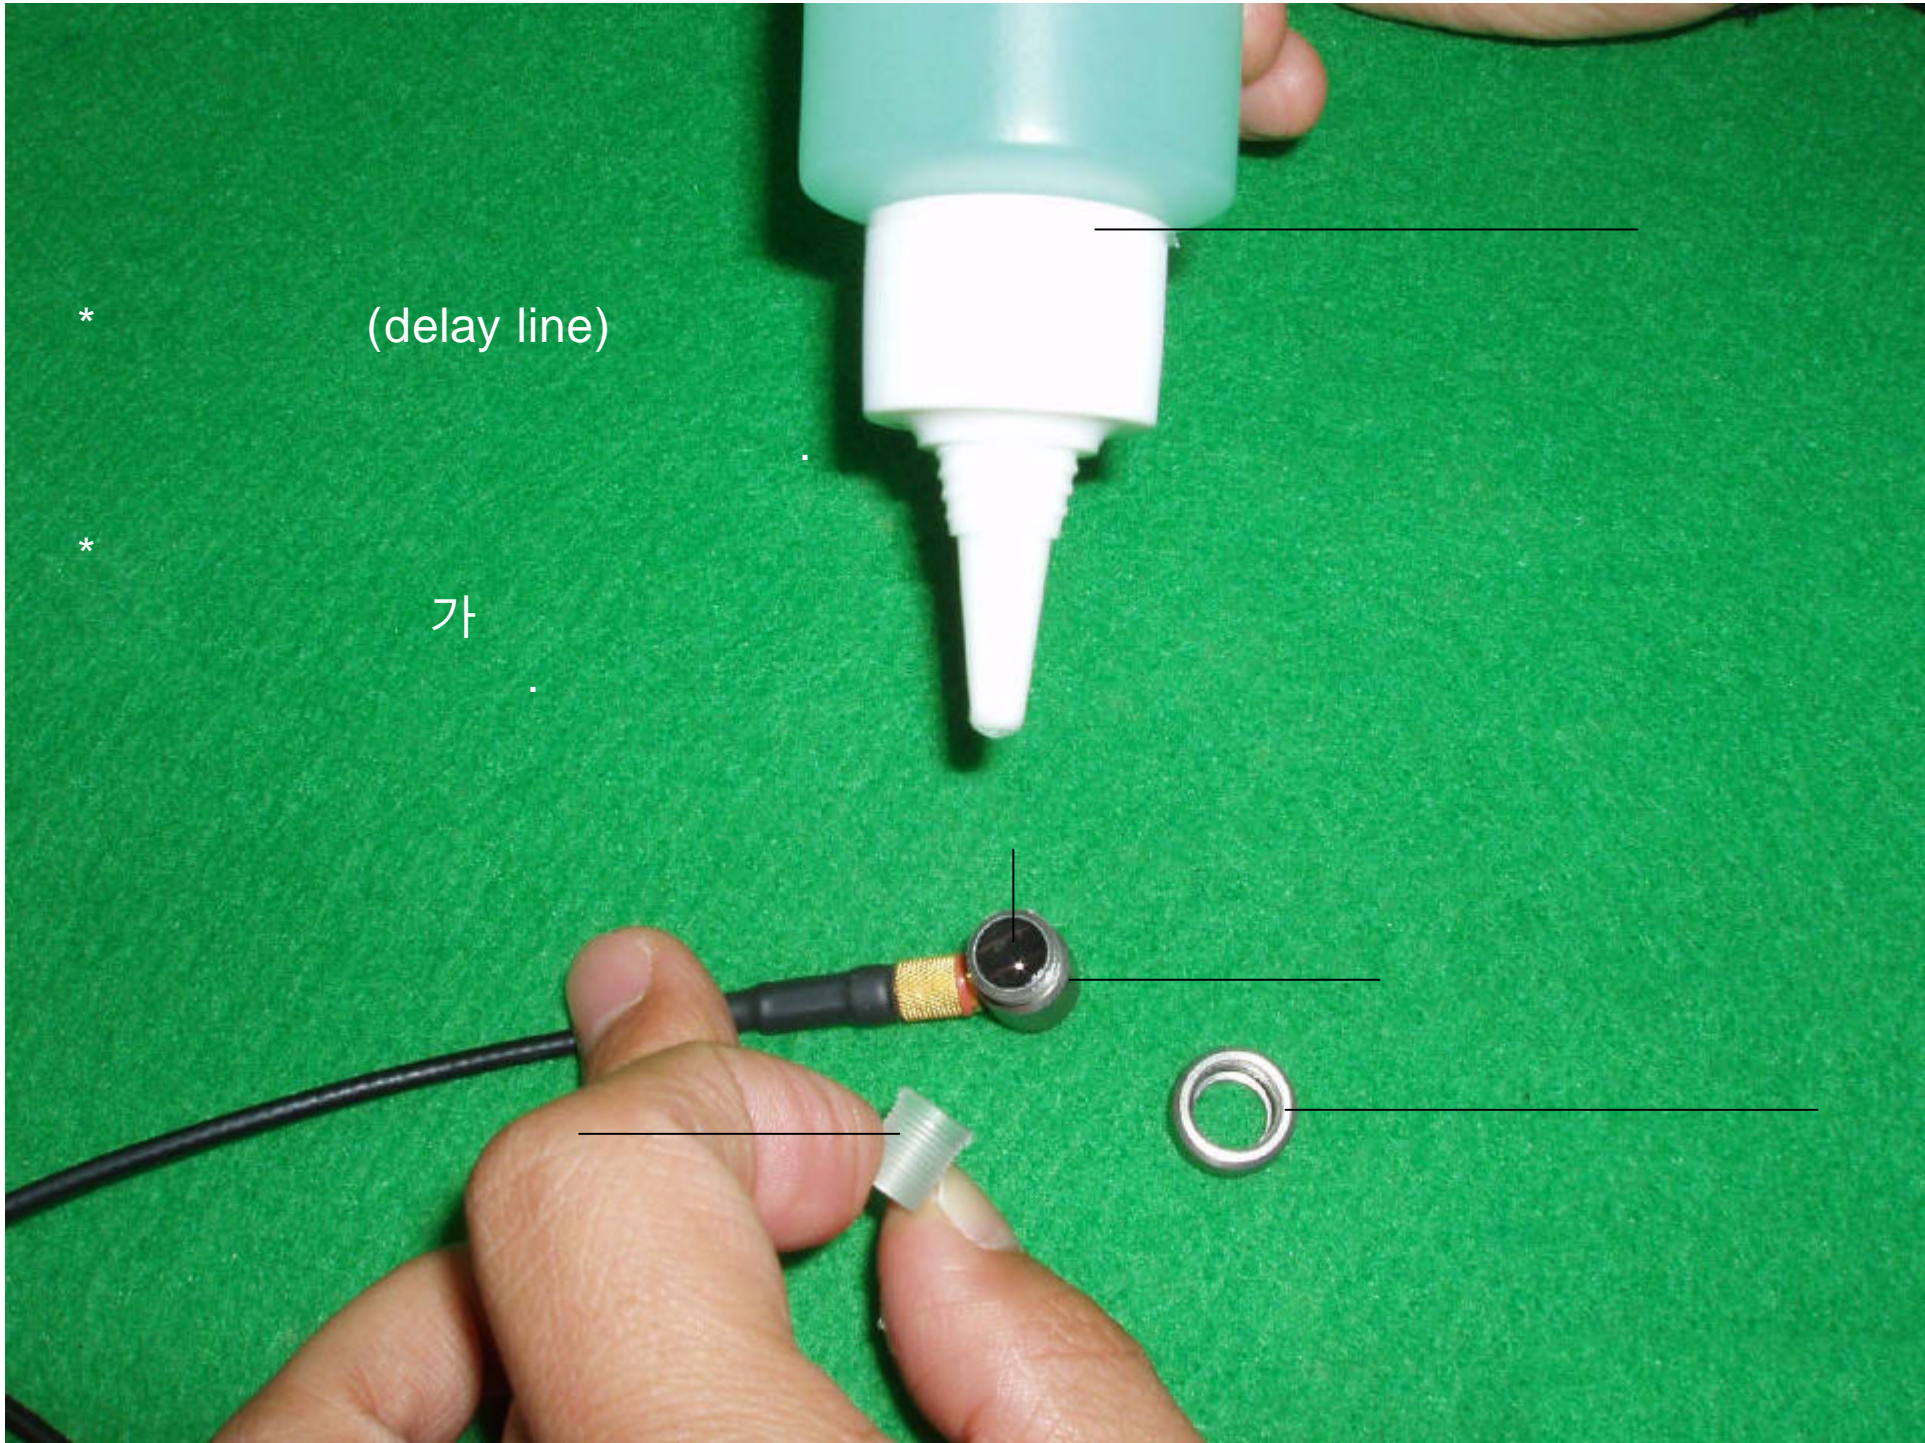

*

(delay line)

*

가

1) E-E:

2) I-E:

3) AUTO: E-E, I-E

4) PLAS:

•

ON/OFF

• ON/OFF

가



ON/OFF

< (Calibration) >



0.63 mm

0.65 mm



< (Calibration)>



< >
1) CAL
2) ,
mm) (, 0.65
mm 가 ,



CAL

< 3) CAL >

6136 m/s

WT Worltech

MM
0.648

ALRM



DIFF

UNIT

SEND

SCAN

IN
MM



ON
OFF

Precision Thickness Gauge



- 가 . DIFF



1.

PLAS

2.

(

)

Ultrasonic Thickness Gauge